

A Novel Compact Electron Spectrometer for Hot Electron Measurement in Pulsed Laser Solid Interaction

H. Chen, P.K. Patel, D.F. Price, B.K Young, P.T. Springer, R. Berry, R. Booth, C. Burns, D. Nelson

This article was submitted to 14th Annual Topical Conference on High Temperature Plasma Diagnostics, Madison, WI, July 8 – 11, 2002

U.S. Department of Energy

Lawrence
Livermore
National
Laboratory

July 5, 2002

DISCLAIMER

This document was prepared as an account of work sponsored by an agency of the United States Government. Neither the United States Government nor the University of California nor any of their employees, makes any warranty, express or implied, or assumes any legal liability or responsibility for the accuracy, completeness, or usefulness of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights. Reference herein to any specific commercial product, process, or service by trade name, trademark, manufacturer, or otherwise, does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States Government or the University of California. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States Government or the University of California, and shall not be used for advertising or product endorsement purposes.

This is a preprint of a paper intended for publication in a journal or proceedings. Since changes may be made before publication, this preprint is made available with the understanding that it will not be cited or reproduced without the permission of the author.

This work was performed under the auspices of the United States Department of Energy by the University of California, Lawrence Livermore National Laboratory under contract No. W-7405-Eng-48.

This report has been reproduced directly from the best available copy.

Available electronically at <http://www.doc.gov/bridge>

Available for a processing fee to U.S. Department of Energy
And its contractors in paper from
U.S. Department of Energy
Office of Scientific and Technical Information
P.O. Box 62
Oak Ridge, TN 37831-0062
Telephone: (865) 576-8401
Facsimile: (865) 576-5728
E-mail: reports@adonis.osti.gov

Available for the sale to the public from
U.S. Department of Commerce
National Technical Information Service
5285 Port Royal Road
Springfield, VA 22161
Telephone: (800) 553-6847
Facsimile: (703) 605-6900
E-mail: orders@ntis.fedworld.gov
Online ordering: <http://www.ntis.gov/ordering.htm>

OR

Lawrence Livermore National Laboratory
Technical Information Department's Digital Library
<http://www.llnl.gov/tid/Library.html>

A novel compact electron spectrometer for hot electron measurement in pulsed laser solid interaction

H. Chen, P. K. Patel, D. F. Price, B. K. Young, P. T. Springer

R. Berry, R. Booth, C. Bruns and D. Nelson

Lawrence Livermore National Laboratory, Livermore, CA 94550-9234, U.S.A.

(July 5, 2002)

Abstract

Ultra-intense laser-matter interactions provide a unique source of temporally short, broad spectrum electrons, which may be utilized in many varied applications. One such, which we are pursuing, is as part of a novel diagnostic to trace magnetic field lines in a magnetically-confined fusion device. An essential aspect of this scheme is to have a detailed characterization of the electron angular and energy distribution. To this effect we designed and constructed a compact electron spectrometer that uses permanent magnets for electron energy dispersion and over 100 scintillating fibers coupled to a 1024x1024 pixel CCD as the detection system. This spectrometer has electron energy coverage from 10 keV to 2 MeV. We tested the spectrometer on a high intensity (10^{17} to 10^{21} W/cm²) short pulse (< 100 fs) laser, JanUSP, at Lawrence Livermore National laboratory using various solid targets. The details of the spectrometer and the experimental results will be reported.

Typeset using REVTeX

I. INTRODUCTION

The characterization of hot electrons produced by ultra-intense laser-matter interactions is not only critical to the understanding of laser plasma physics [1], but also important to many applications making use of the temporally short, broad spectrum of electrons. One of these applications, being pursued at Lawrence Livermore National Laboratory (LLNL) is a novel diagnostic for tracing magnetic field lines in a magnetic fusion device, such as a spheromak [2]. In this scheme a burst of hot electrons is produced by a short pulse laser incident on a solid object (such as an injected pellet), which, after propagating through the magnetic field environment of the fusion device, strikes a wall and produces an observable x-ray signal. An essential aspect of this scheme is to understand the energy and angular distribution of the electrons produced, given certain laser parameters such as laser intensities and prepulse conditions. However, no sufficiently detailed information on the electron production from a thick solid target is presently available: to date, efforts made to obtain the electron production at various laser pulse length and intensities have produced diverse results. These include those measuring the secondary x-rays [3–6] and those directly measuring electrons using magnet-based spectrometers [7,8].

To obtain the required electron production data, we designed and constructed a new Fiber Array Compact Electron Spectrometer (FACES). The spectrometer uses dipole magnets to produce a magnetic field to disperse electrons at different energies. This is the same approach as those direct electron measurements by Malak and Miquel [7] and Gahn et al [8]. In particular, Gahn et al. [8] also used scintillating fibers coupled to a CCD to detect electrons, which is of the same principle as our FACES spectrometer. The instrument reported here is designed to be more compact and versatile with higher energy resolution. In this paper, we describe the design and assembly of the FACES spectrometer, as well as preliminary measurements of the electrons produced with the high intensity ultra-short pulse laser JanUSP at LLNL.

II. SPECTROMETER DESIGN

A schematic of the FACES spectrometer is shown in Fig. 1. Electrons collimated by the slit enter a dipole magnetic field, there they are dispersed energetically along the side where the detection fibers are placed. Stray visible light is blocked by an aluminized mylar foil ($0.2\mu\text{m}$ thickness Al on $0.5\mu\text{m}$ thickness mylar) covering the entrance slit (tantalum, width 8 mm). Fibers are also placed on the back of the spectrometer in the straight-through direction to pick up any signal produced by hard x-rays and γ rays that are not dispersed by the magnetic field.

A uniform magnetic field is generated by permanent magnets sandwiched by two plates of cold rolled steel (area 10 cm by 5 cm). The spacing of the two plates is adjustable to produce an even magnetic strength (less than 5% variations) across the area of interest. We can vary the magnetic field by using magnets of different strengths; for example, magnetic field strengths from 100 to 1000 Gauss will disperse electrons with energies of 10 keV up to several MeV.

For detection, we chose to use scintillating fibers routed to a charge coupled device (CCD). This scheme has several advantages over other detection methods such as silicon diodes or scintillators coupled to photon multipliers. First, with fibers, the spectrometer can have many more channels (increasing the energy resolution). Second, scintillating fibers can be chosen to be relatively insensitive to x-rays and γ rays. The scintillating fibers we employed are polystyrene-based fast green (emission at 492 nm) scintillator (BCF-20) with diameter of 0.5 mm, manufactured by BICRON Saint-Gobain Industrial Ceramics, Inc [9]. They were coated with Extramural Absorber (EMA) to eliminate optical crosstalk. Technical data including scintillating efficiency and transmission efficiency are available from the manufacturer. The fibers are placed 1 mm apart along the sides of the magnets. This corresponds to an energy resolution up to 1%.

We used a 16-bit, water-cooled, 1024×1024 pixel CCD designed and built at LLNL [10,11]. The CCD sensor is a SITe TK1024 [12] with a 1:1 fiber-optical window built in.

A total of 120 individual fluorescing fibers transmit the photons from the electron spectrometer to the surface of the 1 inch square CCD. These were hand loaded and epoxied into a custom designed delrin fiber array holder, then polished to 1 micron level smooth surface. This array was then attached to a spring loaded holder that allowed this polished fiber array to be carefully and accurately coupled to the surface of the CCD without applying any undue pressure to the fiber optical surface at the CCD chip.

The housing of the spectrometer was designed so that the FACES package is as compact as possible. Fig. 2 shows the assembly of the package. The whole spectrometer is placed in a light-tight half-inch thick aluminum box with outermost dimensions of 8.25 inch x 7.25 inch x 3.75 inch. Extreme care has been taken in the design to ensure complete shielding of the spectrometer from possible laser-induced electro-magnetic-pulses (EMP). The aluminum enclosure is then plated with 0.125 inch thick tantalum sheets. As an extremely dense high-Z metal, tantalum shields the spectrometer volume from the stray electrons, high-energy x-rays, γ rays, and other energetic particles generated from the laser-target interactions. The water lines and CCD control are fed through the shielding.

III. EXPERIMENT ON THE JANUSP LASER

We performed experiments on the JanUSP Ti:sapphire laser [13,14]. It has a pulse length of 100 fs and delivers up to 10 J laser energy at 800 nm. The laser is focused with an f/2 parabola to a focus spot size of about $3.5 \mu\text{m}$, and the laser intensity ranges from $10^{17} - 10^{20} \text{W/cm}^2$. The experimental setup inside the JanUSP chamber is shown in Fig. 3. The target for the experiments was high purity iron slab (1 mm thick, 2 mm wide and 50 mm long). The laser is incident on the target at 22.5 degrees off normal. The spectrometer slit is aligned 30 degrees from the laser beam, i.e. 52.5 degrees off normal, and 23 cm away from the target. The chamber is at a vacuum of $\sim 10^{-5}$ torr during these experiments.

We operated the laser in the energy range from 10 mJ to 150 mJ. The magnetic strength of the spectrometer was set to either 150 Gauss or 1000 Gauss, to measure electron energies

up to 1.3 MeV and 6 MeV, respectively. After taking data at each laser shot, we took background data to account for the CCD thermal noise. The background was then subtracted from the signal during data process. To ensure the fiber signals are from the electrons and not other sources, we inverted the magnetic field to deflect the electrons to the side opposite to the electron-dispersion fibers. Under this condition, we detected no signals from the fibers on the dispersion side. From the fibers placed on the side opposite to the entrance slit, in a shot with laser energy of 3 J, we detected a very weak signal from three fibers directly facing the slit. These signal is attributed to hard x-rays and γ rays. There is no observable signal from x-rays and γ rays at ~ 100 mJ laser shots. Further evidence for the spectrometer detecting electrons came from measurements from shots at same laser energies but with different magnet strengths. As shown in Fig. 4, the signal (which is proportional to the number and energy of electrons) shifts along the dispersion plane, corresponding to the dispersion function for the two magnet strengths.

The data processing takes into account the energy absorption by the fibers at different electron energies using data from ESTAR [15]. Fiber scintillating efficiencies and transmission efficiencies are calculated using data provided by the manufacturer [9]. Finally, we took into account the CCD quantum efficiency (15%) and gain (3.7 electrons/count) to derive the number of electrons collected by each fiber whose location corresponds to a given energy. Fig. 5 shows preliminary results from our measurements at a laser energy of 112 mJ. There are a couple of data points that are particularly low counts. This is due to their relatively low fiber efficiency. A more thorough calibration using a known electron source is planned, which will account for these fiber variations and validate the efficiency calculations.

IV. SUMMARY AND FUTURE PLAN

We have described a new fiber-array-based compact electron spectrometer, FACES for measuring the hot electron distribution produced by intense laser-target interactions. Experiments on a short pulse laser prove that the spectrometer is sensitive to these electrons

and insensitive to other forms of high energy radiation produced by the laser. It was designed to be flexible and easy to use and proved to be so. An absolute calibration of the spectrometer is planned which will use a newly built electron gun [16].

Detailed measurements are being obtained on the JanUSP laser, including systematic measurements of electron production from various target materials at different detection angles and laser intensities.

V. ACKNOWLEDGEMENT

The work at the University of California Lawrence Livermore National Laboratory was performed under the auspice of the Department of Energy under Contract No. W-7405-Eng-48. This project was funded by the Laboratory Directed Research and Development (LDRD) Program (01-ER-100).

REFERENCES

- [1] P. Gibbon and E. Forster, Plasma Phys. Control. Fusion **38**, 769 (1996)
- [2] H. McLean, H. Chen, D. Hill, D. Ruytov, this conference.
- [3] G. D. Enright and N. H. Burnett Phys. Rev. A **32**, 3578 (1985)
- [4] M. Schnurer, R. Nolte, T. Schlegel, M. P. Kalachnikov, P. V. Nickles, P. Ambrosi and W. Sandner J. Phys. B **30**, 4653 (1997)
- [5] K. B. Wharton, S. P. Hatchett, S. C. Wilks, M. H. Key, J. D. Moody, V. Yanovsky, A. A. Offenberger, B. A. Hammel, M. D. Perry and C. Joshi Phys. Rev. Lett. **81**, 822 (1998)
- [6] G. Pretzler, Th. Schlegel and E. Fill Phys. Rev. E **62**, 5618 (2000)
- [7] G. Malka and J. L. Miquel, Phys. Rev. Lett, **77**, 75 (1996)
- [8] C. Gahn, G. D. Tsakiris, and K. J. Witte Rev. Sci. Instrum, **71**, 1642 (2000)
- [9] www.bicron.com
- [10] A. D. Conder, J. Dunn, B. K.F. Young Rev. Sci. Instrum. **66**, 709 (1995)
- [11] J. Dunn, B.K.F. Young, A.D. Conder, and R.E. Stewart, in Solid State Sensor Arrays and CCD Cameras, ed. C. N. Anagnostopoulos, M. M. Blouke and M. P. Lesser, SPIE Proceedings, 119 (1996). **2654**, 119 (1996).
- [12] <http://www.site-inc.com/>
- [13] J. D. Bonlie, F. Patterson, D. Price, B. White and P. Springer Appl. Phys. B [Suppl.], **70**, S155 (2000)
- [14] F. Patterson, J. Bonlie, D. Price, B. White, P. Springer, Ultrafast Optics 99 Conference, Ascona, Switzerland, July 11-17, (1999).
- [15] <http://physics.nist.gov/PhysRefData/Star/Text/ESTAR.html>

[16] H. McLean, Private communications

FIGURES

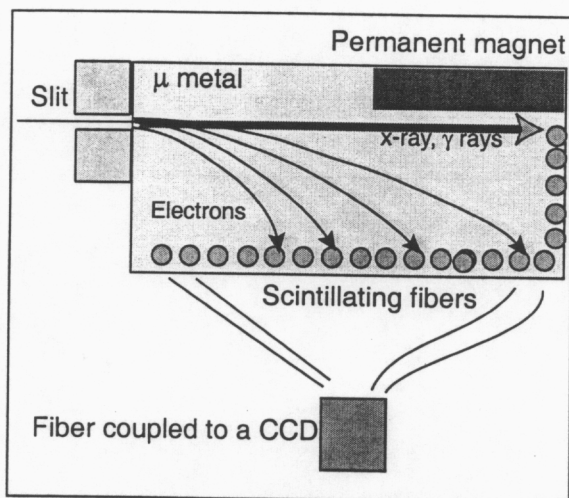


FIG. 1. Schematic diagram of the electron spectrometer.

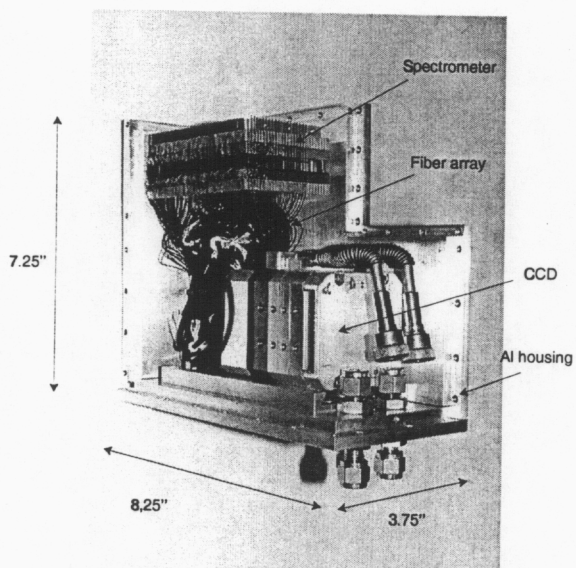


FIG. 2. Photograph of the Fiber Array Compact Electron Spectrometer (FACES). The dimensions are in unit of inches.

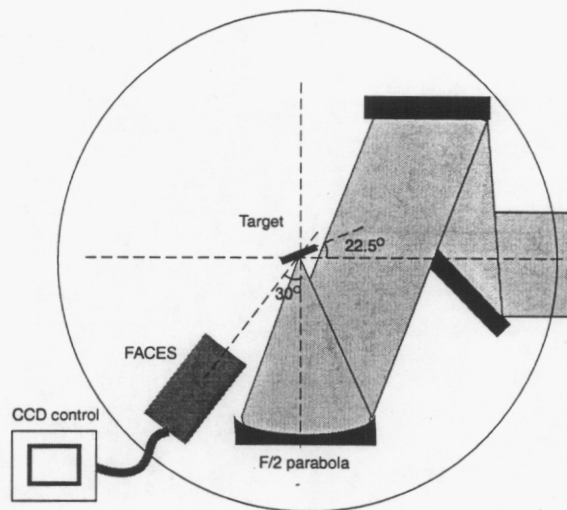


FIG. 3. Diagram of the FACES setup in the JanUSP vacuum chamber.

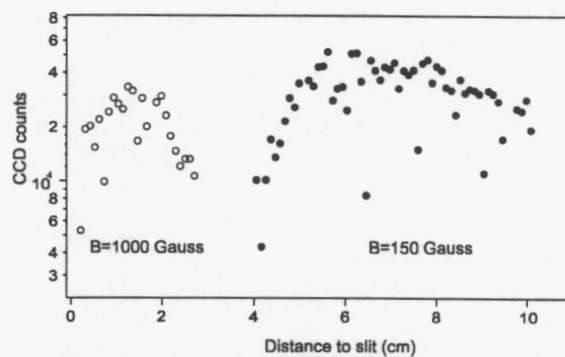


FIG. 4. Signals taken for Fe target at 120 mJ laser energies from two spectrometer magnetic strength setups: 1000 Gauss and 150 Gauss.

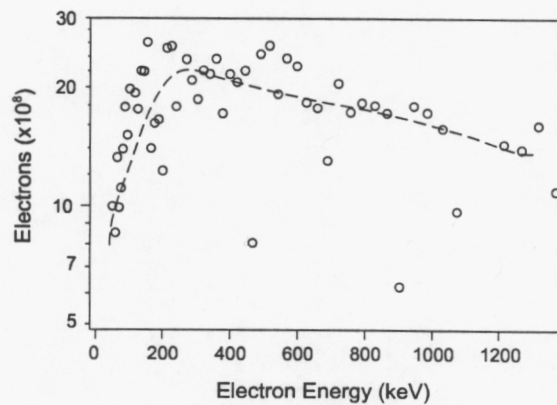


FIG. 5. Electron distribution from a Fe target at 112 mJ laser energy.